

Instructions

FETISH *Fantasy Series*

Thank you for purchasing Fetish Fantasy Series Shock Therapy!
Please read the following instructions before using.

WARNING:

Those who suffer from any of the following conditions or symptoms should refrain from using this device:

- Heart disease
- Pacemaker
- Epilepsy or other neurological disorders
- Pregnant women
- While driving or operating heavy equipment
- Near any metal objects or piercings, including jewelry

Those receiving medical treatment should consult their physician prior to using this device.

CAUTION:

Should you feel any discomfort or abnormality in either the unit or your body, stop use immediately. Do not place the device inside of your mouth.


IN / OUT
Mode Switch



SLOW / FAST
Speed Frequency:
Controls the frequency
of the electronic
current



ON / OFF
Power Dial:
Controls the strength
of the impulse.

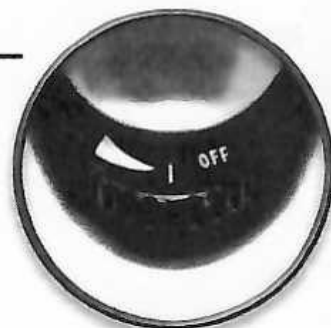


Electrode Jack

Electric Contact



FETISH Shock Therapy Electro Loops

Fantasy Series

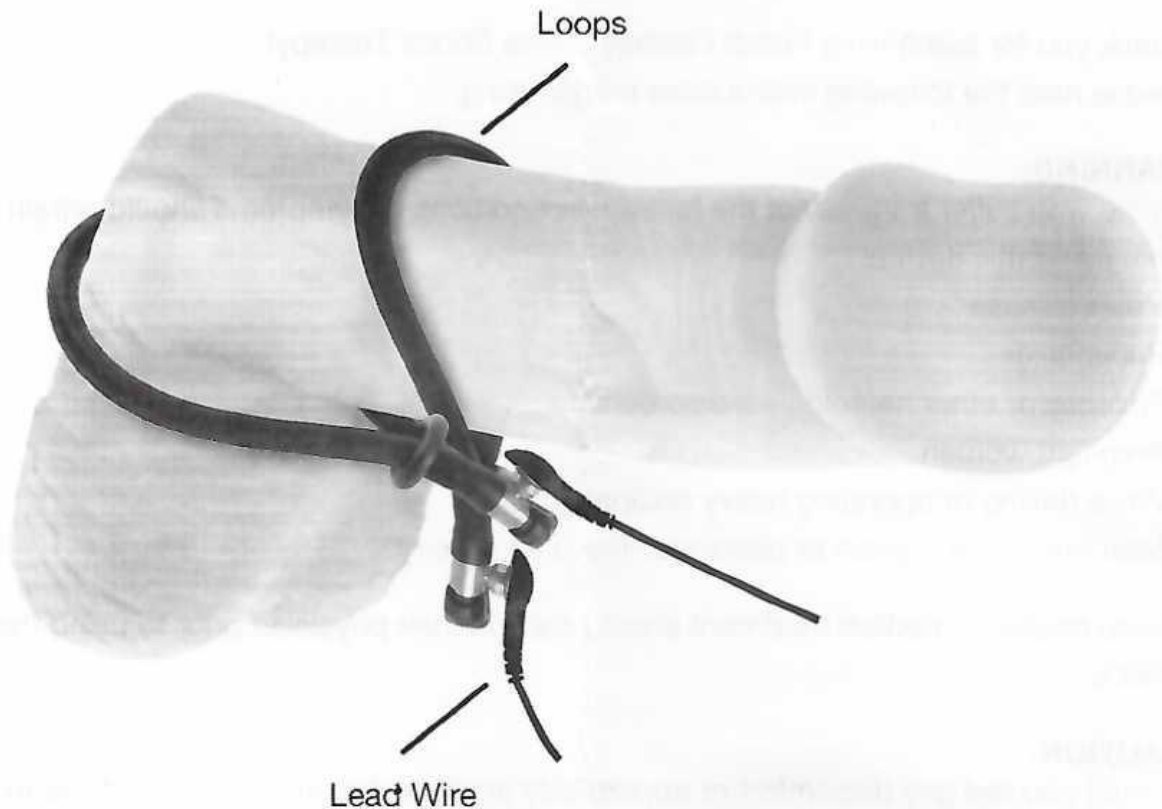

DIRECTIONS:

1. Place the required AAA batteries into the control unit.
2. Snap each lead wire onto the e-stim loops.
3. There are 2 plug-in ports on the power unit. You can use the cuffs and probe simultaneously or separate.
4. Press the “⏻” button to power the unit on.
5. Use the “PULSE”, “TINGLE”, “THROB”, and “INTERVAL” buttons to choose the perfect pulsation pattern.
6. Press the “MODE” button to adjust the speed of the shock.
7. Use the dial to adjust the intensity of the shock.
8. Press the “⏻” button to power the unit off.