

Instructions

FETISH
Fantasy Series

Thank you for purchasing Fetish Fantasy Series Shock Therapy!
Please read the following instructions before using.

WARNING:

Those who suffer from any of the following conditions or symptoms should refrain from using this device:

- Heart disease
- Pacemaker
- Epilepsy or other neurological disorders
- Pregnant women
- While driving or operating heavy equipment
- Near any metal objects or piercings, including jewelry

Those receiving medical treatment should consult their physician prior to using this device.


CAUTION:

Should you feel any discomfort or abnormality in either the unit or your body, stop use immediately. Do not place the device inside of your mouth.

FETISH

Fantasy Series

Shock Therapy Professional Wireless Electro-Massage Kit

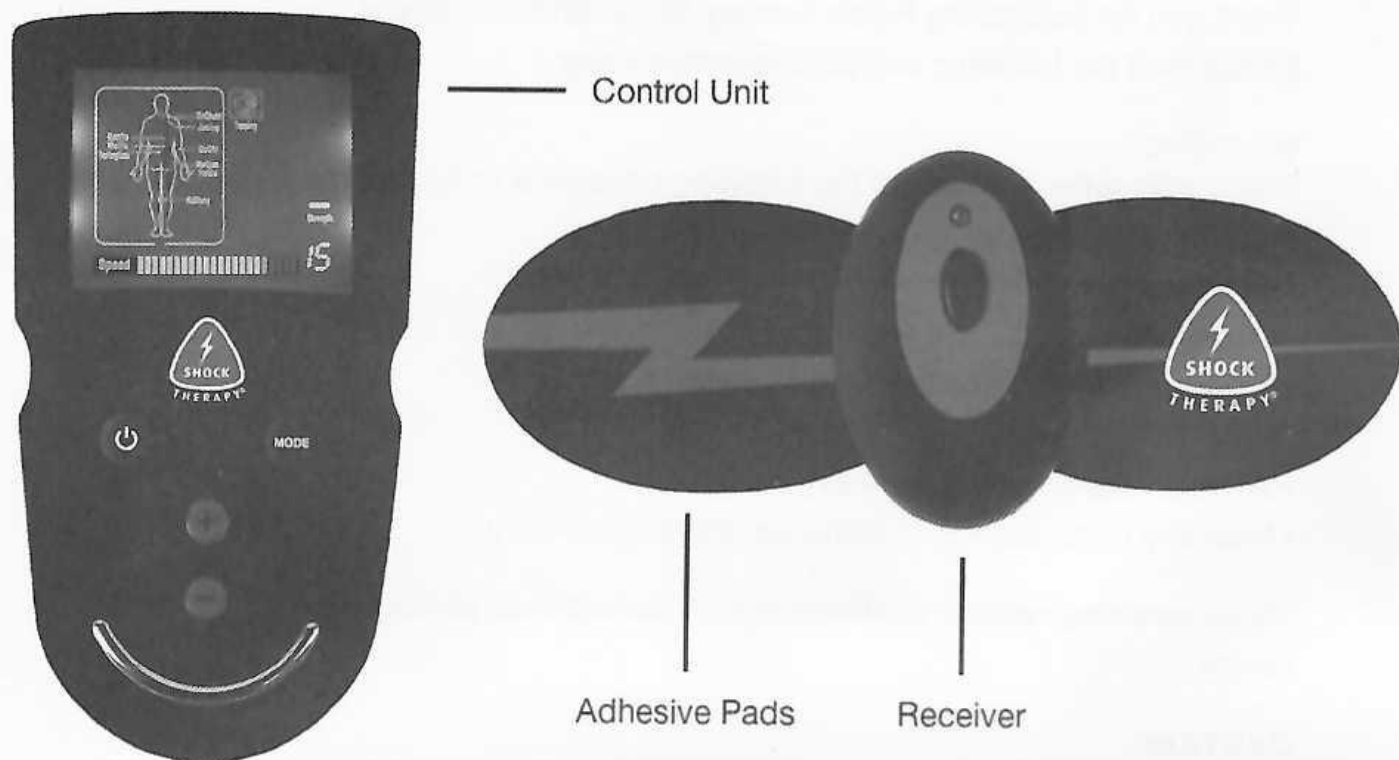

DIRECTIONS:

1. Insert the 2 required AA batteries into the control unit. The batteries should be placed in opposing directions.
2. Insert 1 of the included CR2032 (3V) batteries into each receiver.
3. Attach 1 adhesive pad to each receiver.
4. Place the pad and receiver on the desired pressure point, as shown on the diagram on the control unit's screen.
5. Press the "⏻" button to power the unit on.
6. Cycle through 6 unique pulsation patterns by clicking the "MODE" button.
7. Increase the intensity with the "+" button.
8. Decrease the intensity with the "-" button.
9. Press the "⏻" button to power the unit off.